



## testo · Smart Probes

### Instruction manual



---

# 1 Contents

<b>1</b>	<b>Contents .....</b>	<b>3</b>
<b>2</b>	<b>Safety and the environment.....</b>	<b>5</b>
2.1.	About this document.....	5
2.2.	Ensure safety.....	6
2.2.1.	Safety and the testo 510i .....	6
2.2.2.	Safety and the testo 549i .....	6
2.2.3.	Safety and the testo 805i .....	6
2.3.	Protecting the environment.....	7
<b>3</b>	<b>Specifications .....</b>	<b>7</b>
<b>4</b>	<b>Product description.....</b>	<b>7</b>
4.1.	Overview of Smart Probes.....	7
4.2.	LED status.....	8
<b>5</b>	<b>First steps .....</b>	<b>8</b>
5.1.	Switching on/off.....	8
5.1.1.	Switching on.....	8
5.1.2.	Switching off.....	9
5.2.	Establishing Bluetooth® connection .....	9
5.3.	Transmitting readings .....	9
<b>6</b>	<b>Using the App .....</b>	<b>10</b>
6.1.	Overview of operating controls .....	10
6.2.	App options.....	10
6.2.1.	Set "Language" .....	10
6.2.2.	Display Tutorial .....	11
6.2.3.	Show help .....	11
6.2.4.	Display testo website .....	11
6.2.5.	Display App Info.....	11
6.3.	Application menus .....	11
6.3.1.	Selecting the application menu.....	11
6.3.2.	Setting favourites .....	12
6.3.3.	Displaying information about an application .....	12
6.4.	Displaying Smart Probe details.....	12
6.5.	List, graphic diagram and table view .....	12
6.6.	Settings view .....	13
6.7.	Retaining readings.....	13
6.8.	Exporting readings.....	13
6.8.1.	Excel (CSV) Export .....	13
6.8.2.	PDF Export.....	14
6.8.3.	Exporting a graph.....	14
<b>7</b>	<b>Maintaining the product.....</b>	<b>14</b>

7.1.	Maintaining Smart Probes.....	14
7.2.	Smart Probes App.....	15
<b>8</b>	<b>Tips and assistance .....</b>	<b>15</b>
8.1.	Questions and answers .....	15
8.2.	Accessories and spare parts.....	16
<b>9</b>	<b>Technical data .....</b>	<b>16</b>
9.1.	Bluetooth module .....	16
9.2.	General technical data .....	17
9.2.1.	testo 905i .....	17
9.2.2.	testo 410i .....	18
9.2.3.	testo 405i .....	19
9.2.4.	testo 549i .....	19
9.2.5.	testo 805i .....	20
9.2.6.	testo 605i .....	21
9.2.7.	testo 510i .....	22
9.2.8.	testo 115i .....	23
<b>10</b>	<b>EC Declaration of Conformity .....</b>	<b>24</b>



## 2 Safety and the environment

### 2.1. About this document

#### Use

- > Please read this documentation through carefully and familiarize yourself with the product before putting it to use. Pay particular attention to the safety instructions and warning advice in order to prevent injuries and damage to the products.
- > Keep this document to hand so that you can refer to it when necessary.
- > Hand this documentation on to any subsequent users of the product.

#### Symbols and writing standards

Representation	Explanation
	Warning advice, risk level according to the signal word: <b>Warning!</b> Serious physical injury may occur. <b>Caution!</b> Slight physical injury or damage to the equipment may occur. > Implement the specified precautionary measures.
	Note: Basic or further information.
1. ...	Action: more steps, the sequence must be followed.
2. ...	
> ...	Action: a step or an optional step.
- ...	Result of an action.
<b>Menu</b>	Elements of the instrument, the instrument display or the program interface.
<b>[OK]</b>	Control keys of the instrument or buttons of the program interface.
...   ...	Functions/paths within a menu.
“ ... ”	Example entries

## **2.2. Ensure safety**

- > Do not operate the instrument if there are signs of damage at the housing, mains unit or feed lines.
- > Do not perform contact measurements on non-insulated, live parts.
- > Do not store the product together with solvents. Do not use any desiccants.
- > Carry out only the maintenance and repair work on this instrument that is described in the documentation. Follow the prescribed steps exactly. Use only original spare parts from Testo.
- > Dangers may also arise from the systems being measured or the measuring environment: Note the safety regulations valid in your area when performing the measurements.

### **2.2.1. Safety and the testo 510i**

- Magnetic field
- May be harmful to those with pacemakers.
- > Keep a minimum distance of 10 cm between pacemaker and instrument.

### **2.2.2. Safety and the testo 549i**

- Risk of injury due to pressurized, hot, cold or toxic refrigerants/media!
- > Only to be used by qualified staff.
- > Wear protective goggles and safety gloves.
- > Before applying pressure to the measuring instrument: always fix the instrument tightly onto the pressure connection
- > Comply with the permissible measuring range (0 to 60 bar). Pay particular attention to this in systems with R744 refrigerant, since these are frequently operated at higher pressures!

### **2.2.3. Safety and the testo 805i**

- Laser radiation! Class 2 laser
- > Do not look into the laser beam!

## 2.3. Protecting the environment

- > Dispose of faulty rechargeable batteries/spent batteries in accordance with the valid legal specifications.
- > At the end of its useful life, send the product to the separate collection for electric and electronic devices (observe local regulations) or return the product to Testo for disposal.

## 3 Specifications

Testo Smart Probes are different hand-held measuring instruments for various applications that communicate with your mobile terminal devices by means of an app. The respective Smart Probe performs the measurement and is operated by your mobile terminal device. The various Smart Probes allow you to measure the temperature, humidity, flow, and volume flow at the outlet, or perform pressure, differential pressure, and non-contact temperature measurements in the duct.

## 4 Product description

### 4.1. Overview of Smart Probes



- 1 Measuring unit
- 2 LED
- 3 Key
- 4 Battery compartment (at the back)
- 5 Direction of flow testo 405i / testo 410i (not shown)  
(An arrow on the top of the housing displays the direction of flow in which the measuring instrument has been calibrated and which achieves the best measurement results. Please note the direction of flow during usage.)

4.2. LED status

LED status	Meaning
Flashing red	Low battery status
Flashing yellow	<ul style="list-style-type: none"><li>• Smart Probe is switched on.</li><li>• Smart Probe is searching for a BT connection, but is not connected.</li></ul>
Flashing green	<ul style="list-style-type: none"><li>• Smart Probe is switched on.</li><li>• Bluetooth is connected.</li></ul>

5 First steps

5.1. Switching on/off



5.1.1. Switching on

- 1. Pull the film out of the battery compartment.
- 2. Press the button on your Smart Probe.
  - The Smart Probe switches on.



### 5.1.2. Switching off

1. Press and hold the button on your Smart Probe.
  - The Smart Probe switches off.

## 5.2. Establishing Bluetooth® connection

---



You need a tablet or smartphone with the testo Smart Probes App already installed on it to be able to establish a Bluetooth connection. You can get the App for iOS instruments in the App Store or for Android instruments in the Play Store.

Compatibility:

- requires iOS 8.3 or later/Android 4.3 or later
  - requires Bluetooth 4.0
  - Tested with the following smartphones/tablets:  
[www.testo.com/smartprobesmanuals.html](http://www.testo.com/smartprobesmanuals.html)
- 


- ✓ The testo App Smart Probe is installed on your terminal device and ready for use.
- 1. Press the button on the Smart Probe.
  - The Smart Probe switches on.
  - The LED flashes yellow while connecting via Bluetooth and then flashes green once the connection is established.
  - The connection between the Smart Probe and your mobile terminal device is established.

## 5.3. Transmitting readings

- ✓ The Smart Probe is switched on and connected to your mobile terminal device via Bluetooth.
  - The current readings are automatically displayed in the App.

## 6 Using the App

### 6.1. Overview of operating controls

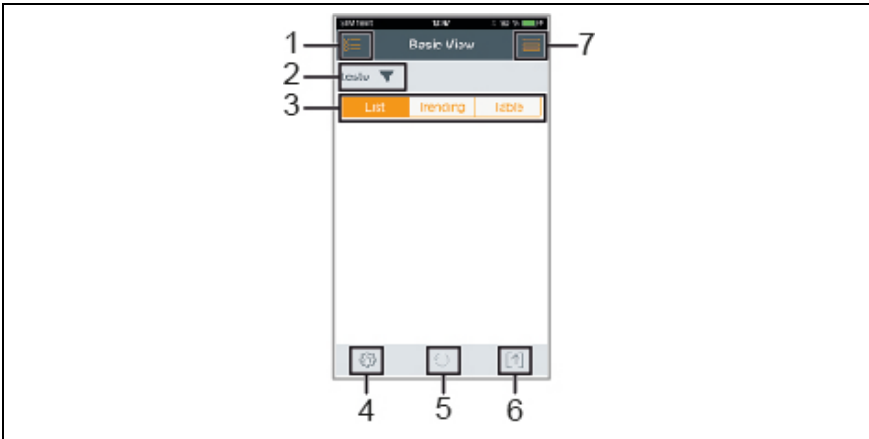

- 1 Choice of applications.
- 2 Display of connected Smart Probes.
- 3 Switch between the views (list, graphic diagram, table)
- 4 Measurement settings. (The menu changes depending on the Smart Probe connected and the application selected)
- 5 Restarts the measuring value recording in graph and table format.
- 6 Export the readings.
- 7 Options menu

## 6.2. App options

### 6.2.1. Set "Language"

1. Tap -> **Settings** -> **Language**.
  - A selection list is displayed.
2. Tap the required language.
  - The selected language receives a green check mark.
3. Tap several times until the measurement view is displayed.
  - The language has been changed.

### 6.2.2. Display Tutorial



The **Tutorial** guides you through the first steps when operating the testo Smart Probes App.

1. Tap -> **Tutorial**
  - The **Tutorial** is displayed. In **Tutorial**, swipe to display the next page.
2. Tap X to close the **Tutorial**.

### 6.2.3. Show help



An internet connection is required to display the testo website.

1. Tap -> **Help**
  - The page [www.testo.com/smartprobesmanuals.html](http://www.testo.com/smartprobesmanuals.html) is displayed.

### 6.2.4. Display testo website



An internet connection is required to display the testo website.

1. Tap -> **About/Link** -> **Testo**
  - The page [www.testo-international.com](http://www.testo-international.com) is displayed.

### 6.2.5. Display App Info



In App Info you can find the version number of the installed App.



1. Tap -> **About/Link** -> **Info**
  - The App's version number is displayed, as well as the ID.
2. Tap ◀ several times until the measurement view is displayed.

## 6.3. Application menus



### 6.3.1. Selecting the application menu

1. Press .
- A selection of menus for various applications is displayed.
2. Select the required application.
- The selection disappears and your selected application is displayed.


### 6.3.2. Setting favourites

1. Press .
- A selection of applications is displayed.
2. Press  next to the application that you would like to designate as a favourite.
- The asterisk is displayed in orange , and the selected application is listed under **Show Favorites**.

### 6.3.3. Displaying information about an application

1. Press .
- A selection of applications is displayed.
2. Press .
- The information about an application is displayed.

## 6.4. Displaying Smart Probe details

- ✓ One or more Smart Probes are connected to your mobile terminal device via Bluetooth.
1. Press .
  - All connected Smart Probes are displayed in this list.
  2. Select the Smart Probe to display the details you would like to see.
  - A list appears with the details for the Smart Probe.
  3. Press **Close** to exit the detailed view.



## 6.5. List, graphic diagram and table view

The available readings can be displayed in different ways in the various views.

- List view  
Displays the readings transmitted by the Smart Probe in the form of a list. Readings from all connected Smart Probes are displayed here.
- Graphic diagram view  
The graphical progression of up to four different readings can be displayed. Tap on a reading above the diagram to select the readings to be displayed.

- **Table view**  
In the Table view, all readings are displayed in sequence according to date and time. The different readings from the individual Smart Probes can be selected by pressing ◀ ▶.

## 6.6. Settings view

1. Press  and select **Edit View**.
- An overview of all Smart Probes and their measurement parameters is displayed.
2. Move the required reading up or down to the position it should be.
3. Press  to hide a Smart Probe reading.
4. Press ▼ to select the unit for a reading.
5. Press **OK** to confirm your settings

## 6.7. Retaining readings

Readings are retained in the “**List**” view; in the “**Trend**” and “**Table**” view, the current readings are still displayed.


- ✓ The Smart Probe is switched on, connected to your mobile terminal device via Bluetooth, and readings are transmitted.
1. Press the button on your Smart Probe.
    - The current reading is retained.
  2. Press the key again.
    - The instrument again displays the current readings.

## 6.8. Exporting readings


### 6.8.1. Excel (CSV) Export

1. Press .
  - A selection of export options appears.
2. Press **Export Excel (CSV)**.
  - A list of readings is displayed.
3. Press .
  - A selection of sending/export options appears.
4. Select your required sending/export options.

### 6.8.2. PDF Export

1. Press .
- A selection of export options appears.
2. Press **Export PDF**.
- A PDF is created and saved on your mobile terminal device (Android only) or sent via e-mail (iOS and Android).
3. Press **Done** to exit the detailed view.

### 6.8.3. Exporting a graph

1. Press .
- A selection of export options appears.
2. Press **Export Graph**.
- An image file of the trend display is created.
3. Press .
- A selection of sending/export options is displayed.
4. Tap on the sending/export option you need.

## 7 Maintaining the product

### 7.1. Maintaining Smart Probes

#### **Cleaning the instrument**

- > Do not use any aggressive cleaning agents or solvents!
- > Mild household cleaning agents or soap suds may be used.
- > If the housing of the instrument is dirty, clean it with a damp cloth.

#### **Keeping connections clean**

- > Keep connections clean and free of grease and other deposits, clean with a damp cloth as required.

#### **Ensuring measuring accuracy**

- > Testo Customer Service would be glad to further assist you if you so wish.
- > Keep within the permissible measuring range!
- > Calibrate instrument regularly (recommendation: once a year).

## 7.2. Smart Probes App

The testo Smart Probes App is kept updated via the Play Store for Android devices and the App Store for iOS devices. Please update the App as soon as a new update is available. We therefore recommend that you do not disable automatic notifications when new updates are available.

# 8 Tips and assistance

## 8.1. Questions and answers

Question	Answer
LED flashes red	<ul style="list-style-type: none"> <li>• Batteries are almost spent.</li> <li>• Change batteries.</li> </ul>
The instrument switches itself off	Remaining battery capacity insufficient > Change the batteries.
--- lights up instead of the measurement parameter display	<ul style="list-style-type: none"> <li>• Outside the permissible measuring range.</li> <li>&gt; Keep within the permissible measuring range.</li> </ul> or <ul style="list-style-type: none"> <li>• Sensor is defective</li> <li>&gt; Contact your testo Service department.</li> </ul>
The App cannot be found in the store	<ul style="list-style-type: none"> <li>• No correct search terms were entered.</li> <li>&gt; Enter an unambiguous search term, e.g.: "testo Smart Probes" or use the link on the testo website.</li> </ul> or <ul style="list-style-type: none"> <li>• Your mobile terminal device does not meet the technical requirements (iOS 8.3 or later, Android 4.3 or later / Bluetooth 4.0 (Low Energy))</li> <li>&gt; Please check the technical data for your mobile terminal device</li> </ul>

## 8.2. Accessories and spare parts

Designation	Item number
testo Smart Case (Refrigeration) for storing and transporting 2 × testo 115i and 2 × testo 549i, dimensions 250 × 180 × 70 mm	0516 0240
testo Smart Case (Heating) for storing and transporting testo 115i, testo 410i, testo 510i, testo 549i and testo 805i, dimensions 250 × 180 × 70 mm	0516 0270
testo Smart Case (VAC) for storing and transporting testo 405i, testo 410i, testo 510i, testo 605i, testo 805i and testo 905i, dimensions 270 × 190 × 60 mm	0516 0250

# 9 Technical data

## 9.1. Bluetooth module



The use of the wireless module is subject to the regulations and stipulations of the respective country of use, and the module may only be used in each case in countries for which a country certification has been granted.

The user and every owner undertake to adhere to these regulations and prerequisites for use, and acknowledge that the re-sale, export, import, etc. in particular in, to or from countries without wireless permits, is their responsibility.

Feature	Values
Bluetooth	Range 15 m (free field) (Varies depending on the capability of the mobile terminal device used.)
Bluetooth type	LSD Science & Technology Co., Ltd L Series BLE module (08 May 2013) <u>based on TI CC254X chip</u>
Qualified Design ID	B016552
Bluetooth radio class	Class 3
Bluetooth company	10274



**Certification**

Austria, Belgium, Bulgaria, Croatia, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Poland, Portugal, Republic of Cyprus, Romania, Slovakia, Slovenia, Spain, Sweden, United Kingdom

**EFTA countries**

Iceland, Liechtenstein, Norway and Switzerland

**Other countries**

USA, Canada, Turkey, Hong Kong

Information from the FCC (Federal Communications Commission)

This instrument complies with part 15 of the FCC Rules. Its commissioning is subject to the following two conditions: (1) This instrument may not cause harmful interference and (2) this instrument must be able to accept interference, even if this could have undesired effects on the operation.

**Changes**

The FCC demands that the user be informed that any changes or modifications to the instrument that have not been explicitly approved by Testo AG may void the user's right to use this instrument.

## 9.2. General technical data



All accuracy specifications apply at a nominal temperature of 22 °C.

### 9.2.1. testo 905i

Feature	Values
Measuring range	-50 to 150 °C / -58 to 302 °F
Accuracy $\pm 1$ digit	$\pm 1$ °C / $\pm 1.8$ °F
Resolution	0.1 °C / 0.1 °F
Measurement rate	1/sec
Available units of measurement	°C, °F
Storage temperature	-20 °C to 60 °C / -4 to 140 °F

Feature	Values
Operating temperature	-20 °C to +50 °C / -4 to 122 °F
Battery type	3 micro batteries AAA
Battery life	250 hrs
Dimensions	222 mm × 30 mm × 24 mm Probe shaft length 100 mm Probe shaft diameter 4 mm
Directives, standards and tests	EU guideline: 2014/30/EU
Warranty	Duration: 2 years Warranty terms: see website <a href="http://www.testo.com/warranty">www.testo.com/warranty</a>

### 9.2.2. testo 410i

Feature	Values
Measuring range	0.4 to 30 m/s / 80 to 5,900 fpm -20 to 60 °C / -4 to 140 °F
Accuracy ± 1 digit	± (0.2 m/s + 2% of m.v.) (0.4 to 20 m/s) ± (40 fpm + 2% of m.v.) (80 to 4,000 fpm) ± 0.5 °C / ±0.9 °F
Resolution	0.1 °C / 0.1 °F 0.1 m/s / 1 fpm
Measurement rate	1/sec
Available units of measurement	°C, °F, m/s, fpm, m³/h, cfm, l/s
Storage temperature	-20 °C to 60 °C / -4 to 140 °F
Operating temperature	-20 °C to +50 °C / -4 to 122 °F
Battery type	3 micro batteries AAA
Battery life	200 hrs
Dimensions	154 mm × 43 mm × 21 mm 40 mm vane diameter
Directives, standards and tests	EU guideline: 2014/30/EU
Warranty	Duration: 2 years Warranty terms: see website <a href="http://www.testo.com/warranty">www.testo.com/warranty</a>

### 9.2.3. testo 405i

Feature	Values
Measuring range <sup>1</sup>	0 to 30 m/s / 0 to 5,900 fpm -20 to 60 °C / -4 to 140 °F
Accuracy ± 1 digit	± (0.1 m/s + 5% of m.v.) (0 to +2 m/s) ± (0.3 m/s + 5% of m.v.) (2 to +15 m/s) ± (20 fpm + 5% of m.v.) (0 to +394 fpm) ± (59 fpm + 5% of m.v.) (394 to +3,000 m/s) ± 0.5 °C / ±0.9 °F
Resolution	0.01 m/s / 1 fpm 0.1 °C / 0.1 °F
Measurement rate	1/sec
Available units of measurement	°C, °F, m/s, fpm, m³/h, cfm, l/s
Storage temperature	-20 °C to 60 °C / -4 to 140 °F
Operating temperature	-20 °C to +50 °C / -4 to 122 °F
Battery type	3 micro batteries AAA
Battery life	15 hrs
Dimensions	200 mm × 30 mm × 41 mm Extendible telescope 400 mm Probe shaft diameter 12 mm Probe tip diameter 9 mm
Directives, standards and tests	EU guideline: 2014/30/EU
Warranty	Duration: 2 years Warranty terms: see website <a href="http://www.testo.com/warranty">www.testo.com/warranty</a>

### 9.2.4. testo 549i

Feature	Values
Measuring range	0 to 60 bar (rel) / 0 to 870 psi (rel)
Overpressure	65 bar
Accuracy ± 1 digit	0.5% of final value of measuring range

<sup>1</sup> Please switch on the Smart Probe in the following ambient conditions: > 10 °C, air velocity 0 m/s = protective cap closed to enable the sensor to heat up.

Feature	Values
Resolution	0.01 bar / 0.1 psi
Measurement rate	2/sec
Available units of measurement	bar, psi, MPa, kPa
Connection	1× 7/16" UNF / 1/4" SAE connection
Overload rel.	65 bar
Storage temperature	-20 °C to 60 °C / -4 to 140 °F
Operating temperature	-20 °C to +50 °C / -4 to 122 °F
Battery type	3 micro batteries AAA
Battery life	150 hrs
Measurable media	CFC, HFC, HCFC, N, H2O, CO2
Dimensions	125 mm × 32 mm × 31 mm
Directives, standards and tests	EU guideline: 2014/30/EU
Warranty	Duration: 2 years Warranty terms: see website <a href="http://www.testo.com/warranty">www.testo.com/warranty</a>

### 9.2.5. testo 805i

Feature	Values
Measuring range	-30 °C to 250 °C / -22 to 482 °F
Accuracy ± 1 digit	± 1.5 °C or ± 1.5% of m.v. (0 to 250 °C) ± 2.0 °C (-20.0 to -0.1 °C) ± 2.5 °C (-30.0 to -20.1 °C)  ± 2.7 °F or ± 1.5% of m.v. (32 to 482 °F) ± 3.6 °F (-4 to 32 °F) ± 4.5 °F (-22 to -4 °F)
Resolution	0.1 °C / 0.1 °F
Measurement rate	2/sec
Available units of measurement	°C, °F
Connection	7/16" – UNF
Storage temperature	-20 °C to 60 °C / -4 to 140 °F

Feature	Values
Operating temperature	-10 °C to +50 °C / 14 to 122 °F
Battery type	3 micro batteries AAA
Battery life	30 hrs
Optics	10:1
Laser marking	Diffraction lens as laser marking (laser circle)
Dimensions	140 mm × 36 mm × 25 mm
Emission level	Adjustable from 0.1 to 1.0
Directives, standards and tests	EU guideline: 2014/30/EU
Warranty	Duration: 2 years Warranty terms: see website <a href="http://www.testo.com/warranty">www.testo.com/warranty</a>

### 9.2.6. testo 605i

Feature	Values
Measuring range	-20 to 60 °C, -4 to 140 °F, 0 to 100% RH
Accuracy ± 1 digit	± 1.8% RH + 3% of m.v. at +25 °C (5 to 80% RH) ± 0.03% RH / K (0 to 60 °C) ± 0.8 °C (-20 to 0 °C) / ± 1.44 °F (-4 to 32 °F) ± 0.5 °C (0 to +60 °C) / ± 0.9 °F (32 to 140 °F)
Resolution	0.1 °F / 0.1 °C 0.1% RH
Measurement rate	1/sec
Available units of measurement	°C, °F, %RH, °Ctd, °Ftd, wetbulb °C, wetbulb °F
Storage temperature	-20 °C to 60 °C / -4 to 140 °F
Operating temperature	-20 °C to +50 °C / -4 to 122 °F

Battery type	3 micro batteries AAA
Battery life	250 hrs
Dimensions	243 mm × 30 mm × 24 mm Probe shaft length 100 mm
Directives, standards and tests	EU guideline: 2014/30/EU
Warranty	Duration: 2 years Warranty terms: see website <a href="http://www.testo.com/warranty">www.testo.com/warranty</a>

### 9.2.7. testo 510i

Feature	Values
Measuring range	0 to 150 hPa / 60 in wc
Accuracy ± 1 digit	± 0.05 hPa (0 to 1.00 hPa) / ± 0.02 in wc (0 to 0.4 in wc)  ± 0.2 hPa + 1.5% of m.v. (1.01 to 150 hPa) ± 0.08 in wc + 1.5% of m.v. (0.41 to 60 in wc)
Overpressure	500 mbar
Resolution	0.01 hPa / 0.01 inch wc
Measurement rate	2/sec
Available units of measurement	mbar, hPa, Pa, mmHg, inHg, in WC, psi, mmWC In conjunction with Pitot tube (optional): m/s, fpm, m³/h, cfm, l/s
Storage temperature	-20 °C to 60 °C / -4 to 140 °F
Operating temperature	-20 °C to +50 °C / -4 to 122 °F
Battery type	3 micro batteries AAA
Battery life	150 hrs
Dimensions	148 × 36 × 23 mm
Directives, standards and tests	EU guideline: 2014/30/EU
Warranty	Duration: 2 years Warranty terms: see website <a href="http://www.testo.com/warranty">www.testo.com/warranty</a>

### 9.2.8. testo 115i

Feature	Values
Measuring range	-40 to 150 °C / -58 to 302 °F
Accuracy ± 1 digit	± 1.3 °C (-20 to 85 °C) ± 2.34 °F (-4 to 185 °F)
Resolution	0.1 °C / 0.1 °F
Measurement rate	1/sec
Available units of measurement	°C, °F
Storage temperature	-20 °C to 60 °C / -4 to 140 °F
Operating temperature	-20 °C to +50 °C / -4 to 122 °F
Battery type	3 micro batteries AAA
Battery life	250 hrs
Dimensions	183 mm × 90 mm × 30 mm max. 35 mm pipe diameter
Directives, standards and tests	EU guideline: 2014/30/EU
Warranty	Duration: 2 years Warranty terms: see website <a href="http://www.testo.com/warranty">www.testo.com/warranty</a>

# 10 EC Declaration of Conformity



Declaration No.  
0006 / 2015

Wir messen es.



## EG-Konformitätserklärung EC declaration of conformity

Für die nachfolgend bezeichneten Produkte:  
*We confirm that the following products:*

**testo 405i / testo 410i**  
**testo 510i / testo 549i**  
**testo 605i / testo 115i**  
**testo 905i**

Best. Nr.: / Order No.: 0560 1405 / 0560 1410  
Best. Nr.: / Order No.: 0560 1510 / 0560 1549  
Best. Nr.: / Order No.: 0560 1605 / 0560 1105  
Best. Nr.: / Order No.: 0560 1905

wird bestätigt, daß sie den wesentlichen Schutzanforderungen entsprechen und bei bestimmungsmäßiger Verwendung den grundlegenden Anforderungen folgender Richtlinie entsprechen:

*corresponds with the main protection requirements and, if used according to their intended purpose, comply with the essential requirements of the directive:*

### Richtlinien / directives

- ☒ R&TTE 199/5/EG (bis/until 13.06.2016)
- ☒ RED 2014/53/EU (ab/from 14.06.2016)

Zur Beurteilung der Erzeugnisse wurden folgende Normen herangezogen:  
*For assessment of the product following standards have been called upon:*

### Normen / standards

- ☒ EN 301 489-1 V1.9.2: 2011
- ☒ EN 62479:2010
- ☒ EN 301 489-17 V2.2.1: 2012
- ☒ EN 60950-1:2006+A11:2009+A1:2010+A12:2011+A2:2013
- ☒ EN 300 328 V1.8.1: 2012

Diese Erklärung wird für: / *This declaration is given in responsibility for:*

**Testo AG**  
**Postfach / P.O. Box 1140**  
**79849 Lenzkirch / Germany**  
**[www.testo.com](http://www.testo.com)**

abgegeben durch / *by:*

Dr. Rolf Merte  
(Name / name)

Wolfgang Schwörer  
(Name / name)

Head of Research & Development  
(Stellung im Betrieb des Herstellers)  
(Position in the company of the manufacturer)

Head of Firmware & Electronics  
(Stellung im Betrieb des Herstellers)  
(Position in the company of the manufacturer)

Lenzkirch, 11.11.2015  
(Ort, Datum / place, date)

ppa  
(Rechtsgültige Unterschrift)  
(Legally valid signature)

i.V.  
(Rechtsgültige Unterschrift)  
(Legally valid signature)





Declaration No.  
0007 / 2015

Wir messen es.



## **EG-Konformitätserklärung** **EC declaration of conformity**

Für die nachfolgend bezeichneten Produkte:  
*We confirm that the following products:*

**testo 805i**

Best. Nr.: / Order No.: 0560 1805

wird bestätigt, daß sie den wesentlichen Schutzanforderungen entsprechen und bei bestimmungsmäßiger Verwendung den grundlegenden Anforderungen folgender Richtlinie entsprechen:

*corresponds with the main protection requirements and, if used according to their intended purpose, comply with the essential requirements of the directive:*

### **Richtlinien / directives**

- ☒ **R&TTE 199/5/EG** (bis/until 13.06.2016)  
☒ **RED 2014/53/EU** (ab/from 14.06.2016)

Zur Beurteilung der Erzeugnisse wurden folgende Normen herangezogen:  
*For assessment of the product following standards have been called upon:*

### **Normen / standards**

- |   |  |
|---|--|
| <input checked="" type="checkbox"/> <b>EN 301 489-1 V1.9.2: 2011</b>  | <input checked="" type="checkbox"/> <b>EN 62479:2010</b>                                     |
| <input checked="" type="checkbox"/> <b>EN 301 489-17 V2.2.1: 2012</b> | <input checked="" type="checkbox"/> <b>EN 60950-1:2006+A11:2009+A1:2010+A12:2011+A2:2013</b> |
| <input checked="" type="checkbox"/> <b>EN 300 328 V1.8.1: 2012</b>    | <input checked="" type="checkbox"/> <b>EN 60825-1:2007</b>                                   |

Diese Erklärung wird für: / *This declaration is given in responsibility for.*

**Testo AG**  
**Postfach / P.O. Box 1140**  
**79849 Lenzkirch / Germany**  
**[www.testo.com](http://www.testo.com)**

abgegeben durch / *by:*

Dr. Rolf Merte  
(Name / name)

Wolfgang Schwörer  
(Name / name)

Head of Research & Development  
(Stellung im Betrieb des Herstellers)  
(Position in the company of the manufacturer)

Head of Firmware & Electronics  
(Stellung im Betrieb des Herstellers)  
(Position in the company of the manufacturer)

Lenzkirch, 11.11.2015  
(Ort, Datum / place, date)

ppa  
(Rechtsgültige Unterschrift)  
(Legally valid signature)

i.V.  
(Rechtsgültige Unterschrift)  
(Legally valid signature)

