



Specificatie & Configuratie

Naam apparaat: Kt1LcdMu-T
Type apparaat: Multi-use Int.Temp.
Serienummer: LM660033
Tijdzone: GMT:+1 Zomertijd
Firmwareversie: 1.14F
Tripnummer: 1
Trips resterend: Meerdere
Temp.eenheid: Celsius
Temp.bereik: -40 to +80°C
Batterij: 3.00V - 100%
Aantal reg.'s: 960
Interval: 00:01:00
Startuitstel: 0 sec
Starttijd: 29/06/16 17:00
Stoptijd: Niet ingesteld




Alarm (Tijd boven/onder Alarm)

Type:	Temp.	Max. non-stop	Max. totaal	Buiten spec.
EH:	n/a			
H:	n/a			
L:	n/a			
EL:	n/a			

Samenvatting/Statistieken Bestand gemaakt op: 30/06/16 11:11:14

Maximumtemperatuur:	+60.14°C	Status:	Stopped
Minimumtemperatuur:	-39.00°C	Tripduur:	16:00:00
Gem. temperatuur:	+14.20°C	Tijd binnen spec.:	16:00:00
Mean Kinetic Temp.:	+52.97°C	Gestart op:	29/06/16 17:00:00
Actieve markeringen:	0	Gestopt op:	30/06/16 08:59:00
Gestart door:	Start timer	Gebruikt geheugen:	1% 960/48632
Gestopt door:	#Records reached		

Omschrijving: Calibration

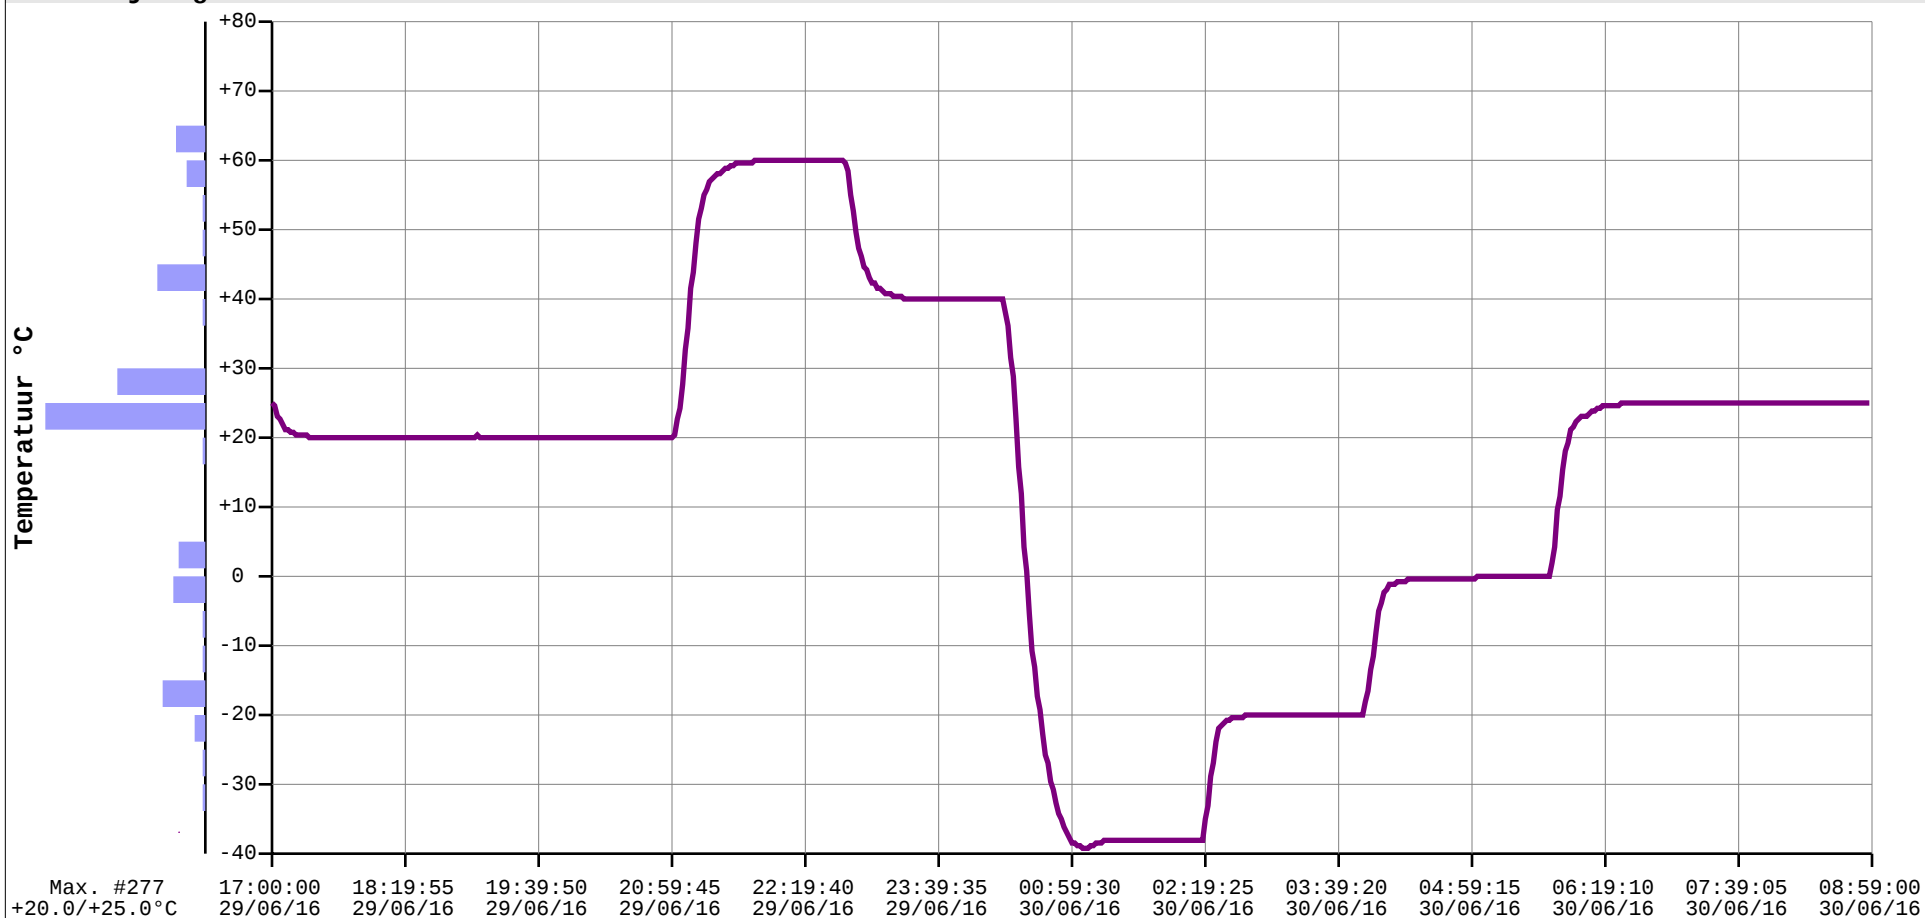

#Registraties

Tijd/datum (dd/mm/jj)

Notities:

This Kt1LcdMu-T with an accuracy of $\pm 0.3^{\circ}\text{C}$ from -40°C to $+80^{\circ}\text{C}$ ($\pm 0.6^{\circ}\text{F}$ from -40°F to $+176^{\circ}\text{F}$) and an resolution of 0.01°C ($^{\circ}\text{F}$) has been calibrated in the calibration chamber of Askey Dataloggers.
The reference equipment used is traceable to National Institute of Standards and Technology. Device: #LM660033